




OneVue Sense

Temperature Probe with CertiTrak™

Simply the easiest way to maintain the accuracy of the calibrated probes in all your temperature monitoring environments.

Documentation of probe calibration to NIST standards, as well as probe replacement policies and procedures, is required by the CDC and other authorities having jurisdiction (AHJs). Our Temperature Probe with CertiTrak Calibration Certification Tracking eliminates the need to manually track calibration data and probe life of your temperature monitoring probes.

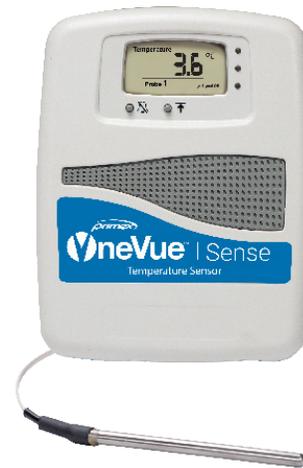

Temperature Probe with CertiTrak

Using patent-pending technology, each probe activates CertiTrak when the probe is initially inserted into a OneVue Sense Temperature Sensor and put into service.

PRIMEXPROBE WITH CERTITRAK	
Part No.	Description
T100SMRT	CertiTrak Probe
SMRTGRP-C	Solid Wax Based Thermobuffer (assembled with T100SMRT probe)
SMRTGRP-G	Glycol Thermobuffer (assembled with T100SMRT probe)

>> CertiTrak links a unique Certificate of Traceability and Calibration Testing to each individual probe within OneVue Monitor software. The certificate provides all the data required for compliance to guidelines issued by the CDC and other authorities having jurisdiction.

>> A record of the last calibration testing date for the individual

probe, the date it was put into service and the days until the next calibration testing is due (or probe replacement) are all linked to the probe record in OneVue Monitor.

>> The unique Certificate of Traceability and Calibration Testing (Calibration Data Report) is available with just one click on the probe serial number.

Calibration Data Report					
Tested For:		Primex, Inc.		Calibration Equipment Used	
Model Number:	Q13790-1	Manufacturer:	Agilent	Model Number:	34410A
Serial Number:	598659-193	Serial Number:	MY53007340	Calibration date:	2/5/2014
Sales Number:	375397	Due date:	2/5/2015	Manufacturer:	Omega
Test Date:	1/30/2015	Model Number:	DP95	Serial Number:	T2543-9167
		Calibration date:	1/8/2015	Calibration date:	1/8/2015
		Due date:	1/8/2016	Due date:	1/8/2016

Temperature Data					
Thermometer (Deg.C)	Actual Probe Resistance	Actual Probe Temperature (°C)	Temperature Deviation (°C)	Calibration Expanded Uncertainty: k=2 (°C)	Pass/Fail
-18.43	928.50	-18.25	0.18	±0.388	PASS
38.77	1151.10	38.88	0.11	±0.288	PASS

Probe Life

Probe Serial No. [4775-1000](#)

Last Testing Date 2013-01-02

First Use Date 2015-10-26

Edit Account

Name *

Street Address 1

Street Address 2

Zip Code

City

State

Country

Time Zone

NTP Server 1

NTP Server 2

NTP Server 3

Use Session Timeout

Session Timeout

Probe Re-Certification

Re-Certify On

>> A Probe Replacement Status Report makes it easy to plan when to change out a probe, allowing you to manage inventory and replacement costs more effectively.

Probe Replacement - Verona Office									
Probe Serial Number	Asset Name	Sensor Name	Business Unit	Location	Gateway ID	First Use Date	Last Testing Date	Probe Recertification	Days To Recertification
4775-1000	Basement Freezer	Temperature-66.8A-1	Research & Development	Lab	00:1E:B3:01:66:8A	2015-10-26 08:32:14 PM	2013-01-02	First Use Date	365

To Learn More:
 Call: 855-557-0337
 Email: info@primexinc.com

primexinc.com



OneVue is a trademark of Primex. The innovative technology software solution for facility and time synchronization monitoring and reporting. All other trademarks are the property of their respective owners.

©2020 Primex. The Primex logo is a registered trademark of Primex. All Rights Reserved. 2.22.2020